



Admelog® SoloStar® (insulin lispro injection) 100 units/mL

Admelog SoloStar Insulin Pen Parts:

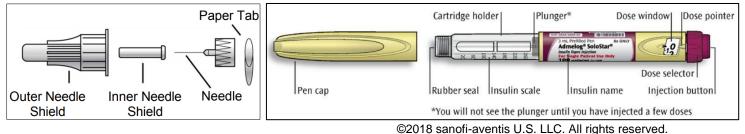

Where to inject:

- Rotate injections between injection spots #1-4:
 - 1. **Stomach**, except for the 2-inches around the belly button
 - 2. Top and outside of **thighs**, except in the bony area close to the knees
 - 3. Back of the **upper arms** (might work best if someone else is injecting)
 - 4. Top and outside of the **buttocks**
- Insulin is injected into the layer of fatty tissue under the skin, not into the muscle
- Do **not** inject into the same spot every time
- Do **not** inject into moles or scars

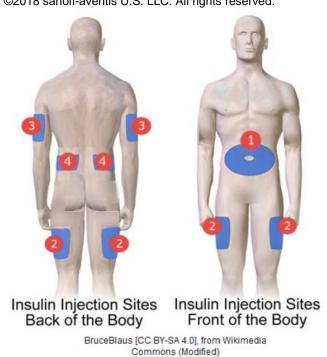

Prepare to inject:


- 1. If your Admelog SoloStar pen is in the refrigerator, take it out at least 1-2 hours before use
- 2. Check the label to make sure you are using the right insulin pen
- 3. Check the expiration date
- 4. Remove the pen cap to check the insulin
 - Do **not** use insulin that is cloudy or not clear, or if it has any specks

Department of Pharmacy/Pediatric Endocrinology

Step 1 Check The insulin

Step 2 Attach The needle	 5. Wipe the pen tip with an alcohol pad 6. Remove the seal on the needle cap Do not share needles or insulin pens with anyone else Do not re-use needles 7. Twist or push (based on the needle type) the needle straight onto the pen tip
Step 3 Perform A safety test	 For each injection: 1. Select a dose of 2 units 2. Take off the outer needle cap (save it) and inner needle cap (throw it away) 3. With the pen pointing up, tap the insulin to move the air bubbles to the top

- 4. Press the button all the way in and make sure insulin comes out of the needle
 - Repeat up to two more times with the same needle if needed
 - If insulin does not come out after three times, change the needle and try again
 - If insulin still does not come out after changing the needle, the pen may be broken

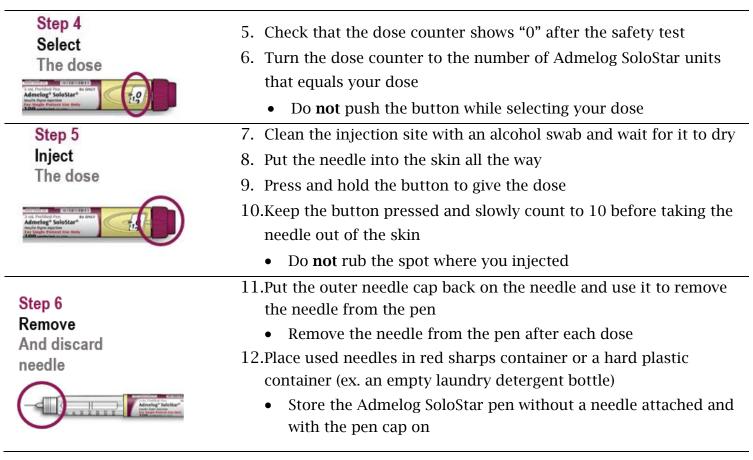

Department of Pharmacy/Pediatric Endocrinology Admelog® SoloStar® (insulin lispro injection) 100 units/mL

Where to store Admelog SoloStar:

- Unused pens should be kept in the refrigerator
- Open or in-use pens should be kept at room temperature for a maximum of 28 days
- After 28 days, Admelog SoloStar pens should be thrown away - even if there is leftover insulin
- Do **not** keep Admelog SoloStar where there is direct heat or direct light
- If Admelog SoloStar is frozen or overheated, throw it away

Top five tips for using your insulin:

- 1. Use Admelog SoloStar before meals and snacks, as directed
- 2. Rotate your injections between the four injection spots listed above
- Always use a new needle for each injection and clean the injection site before each dose
- 4. Slowly count to 10 after pressing the dose button
- If insulin leaks after the injection, do not re-dose; be sure to keep the needle in the skin for at least 10 seconds next time

If you would like more information on how to inject insulin using your Admelog SoloStar, you can visit:

https://www.admelog.com/how-to-use-admelog



Disclaimer: This document contains information and/or instructional materials developed by Michigan Medicine for the typical patient with your condition. It may include links to online content that was not created by Michigan Medicine and for which Michigan Medicine does not assume responsibility. It does not replace medical advice from your health care provider because your experience may differ from that of the typical patient. Talk to your health care provider if you have any questions about this document, your condition or your treatment plan.

Patient Education by <u>Michigan Medicine</u> is licensed under a <u>Creative Commons Attribution</u> <u>NonCommercial-ShareAlike 4.0 International Public License</u>. Last Revised 01/2019