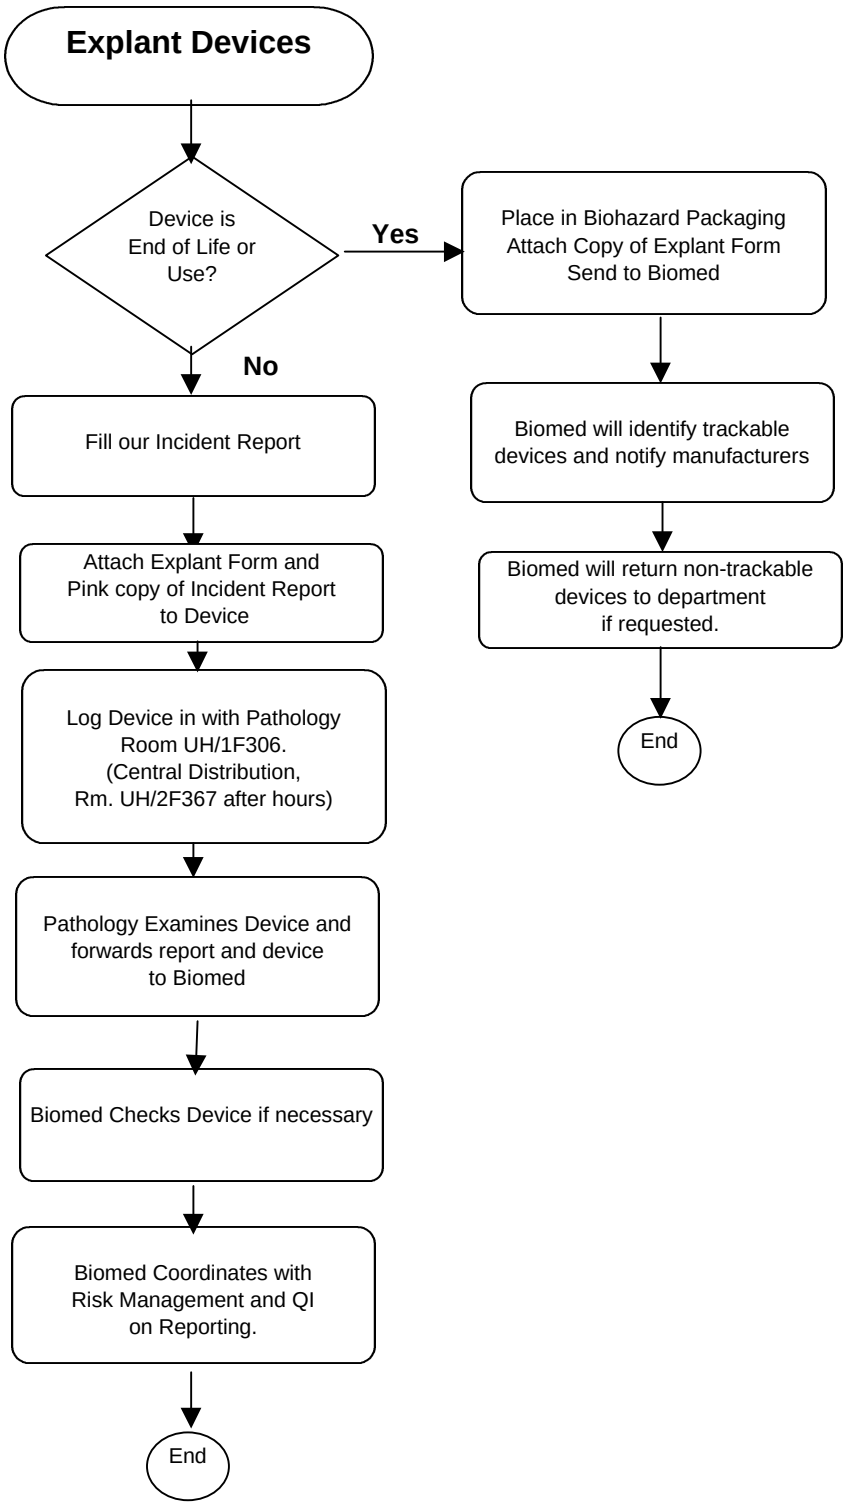
Explant Devices
Device is End of Life or Use?
Yes
No
Place in Biohazard Packaging Attach Copy of Explant Form Send to Biomed
Biomed will identify trackable devices and notify manufacturers
Biomed will return non-trackable devices to department if requested.
End
Fill our Incident Report
Attach Explant Form and Pink copy of Incident Report to Device
Log Device in with Pathology Room UH/1F306. (Central Distribution, Rm. UH/2F367 after hours)
Pathology Examines Device and forwards report and device to Biomed
Biomed Checks Device if necessary
Biomed Coordinates with Risk Management and QI on Reporting.
End