




MEDEQUIP
HOME CARE SERVICES

UNIVERSITY OF MICHIGAN
HEALTH SYSTEM


Oxygen Concentrator Tubing Assembly- Adult (No Humidification)

How do I connect my nasal cannula and tubing to my concentrator?

Step 1: Connect your nasal cannula to the tubing swivel connector

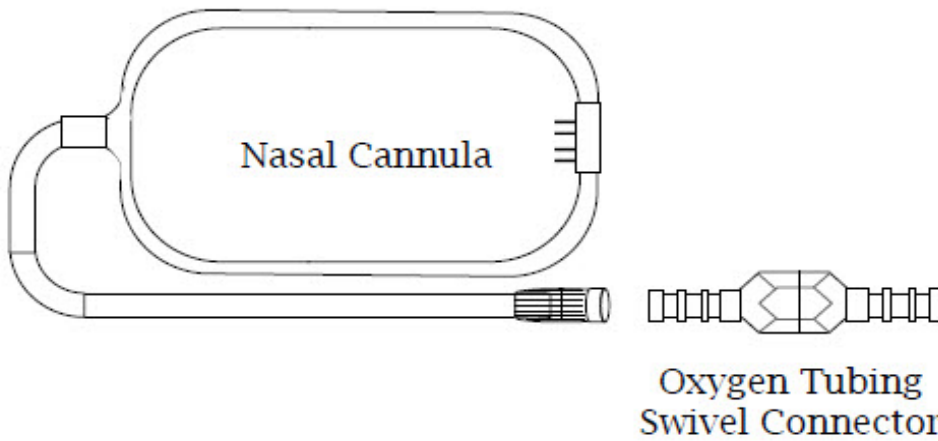


Step 2: Connect your swivel connector to your tubing

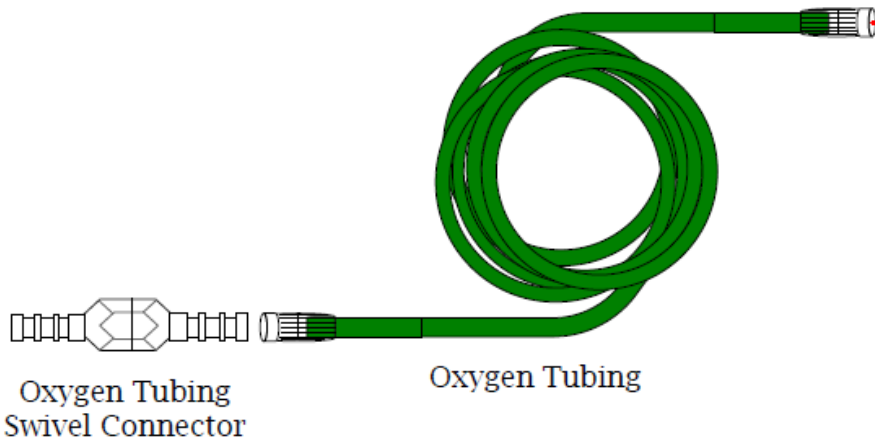


Home Care Services, MedEQUIP
(800) 530-0714

Step 3: Connect your oxygen tubing to the concentrator

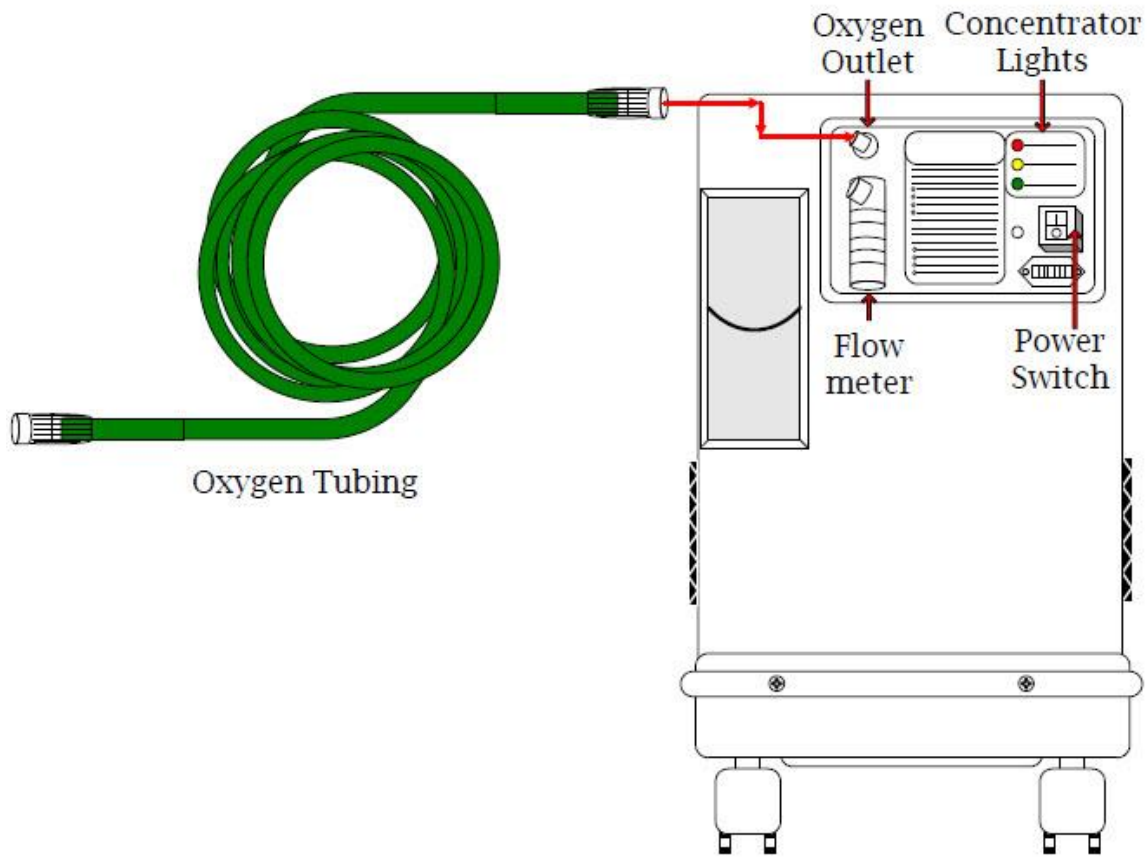

Step 4: Total unit connection

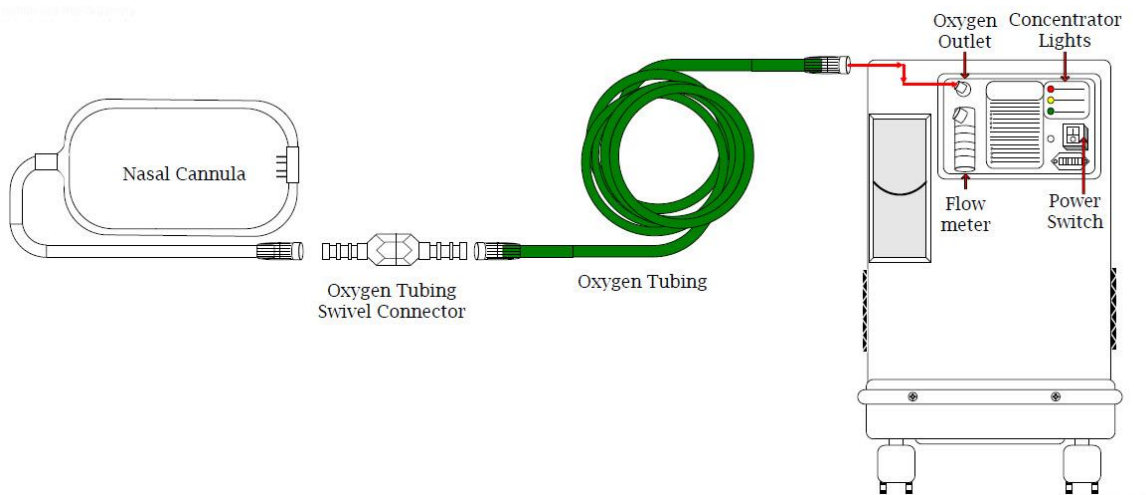

How often should I change my supplies?

Schedule for Change/Cleaning Patient Use Items		
Product #	Description	Changing Schedule
2025G	Oxygen Tubing 25ft	Change Every 3 Months
2050G	Oxygen Tubing 50ft	Change Every 3 Months
1600	Nasal Cannula Adult 7ft	Change Every 2 Weeks
1220	Oxygen Tubing Swivel Connector	Change Every 3 Months
Wipe and clean nasal cannula with damp cloth twice daily		

What indicator lights do I need to know on my concentrator?



Concentrator Lights	
● RED	Call the Supplier
● YELLOW	Low Oxygen Purity
● GREEN	Normal Oxygen

Disclaimer: This document contains information and/or instructional materials developed by the University of Michigan Health System (UMHS) for the typical patient with your condition. It may include links to online content that was not created by UMHS and for which UMHS does not assume responsibility. It does not replace medical advice from your health care provider because your experience may differ from that of the typical patient. Talk to your health care provider if you have any questions about this document, your condition or your treatment plan.

Author: Rachel Stout, Garret Fugitt, RRT, LRT, Brad Hayden
 Reviewers: Sarah Middlemas, MPH

Patient Education by [University of Michigan Health System](http://www.umhs.edu) is licensed under a [Creative Commons Attribution-NonCommercial-ShareAlike 3.0 Unported License](https://creativecommons.org/licenses/by-nc-sa/3.0/). Last Revised 02/2016